

CERTIFICATE OF ANALYSIS

PRODUCT ARGIRELINE® peptide solution C
CODE P06-PD010
BATCH F313/20

ANALYTICAL BULLETIN

TEST	SPECIFICATION	RESULT	METHOD
Physical appearance	Translucent solution	Correct	CC-10-01-B6
Colour	Colourless	Correct	CC-10-01-B6
Specific gravity	-	-	
pH	3.0-6.0	5.3	CC-10-01-B1
Viscosity (cPs) ¹	-	-	
Particle size (mm)	-	-	
Refractive index	-	-	
Dry residue (%)	-	-	
Identification (HPLC)	Similar retention time as in house ref.standard	Correct	CC-10-01-B19

MICROBIAL TEST

Total aerobic microbial count	<100 cfu/g	Correct	MI-10-01-D09
Total yeast and mould count	<10 cfu/g	Correct	MI-10-01-D09
<i>Escherichia coli</i>	Absence/0.5g	Correct	MI-10-01-D09
<i>Pseudomonas aeruginosa</i>	Absence/g	Correct	MI-10-01-D09
<i>Staphylococcus aureus</i>	Absence/g	Correct	MI-10-01-D09
<i>Candida albicans</i>	Absence/g	Correct	MI-10-01-D09

Manufacturing date: 04/20
Retest date: 04/22

Approved on: 22/04/2020



QUALITY CONTROL
Anna Casadó



QUALITY ASSURANCE
Dr. Fernando Fernández

Printed on: 23/06/2020

FG-10-01/2 v.2

Sample Name

ID

Data Filename

Date Acquired

Column


: ARGIRELINE® peptide solution C

: P06-PD010 F313/20

: 17042020P06-PD010.19.lcd

: 18/04/2020 5:51:41

: Kromasil 100-5C8, 250 x 4.6 mm

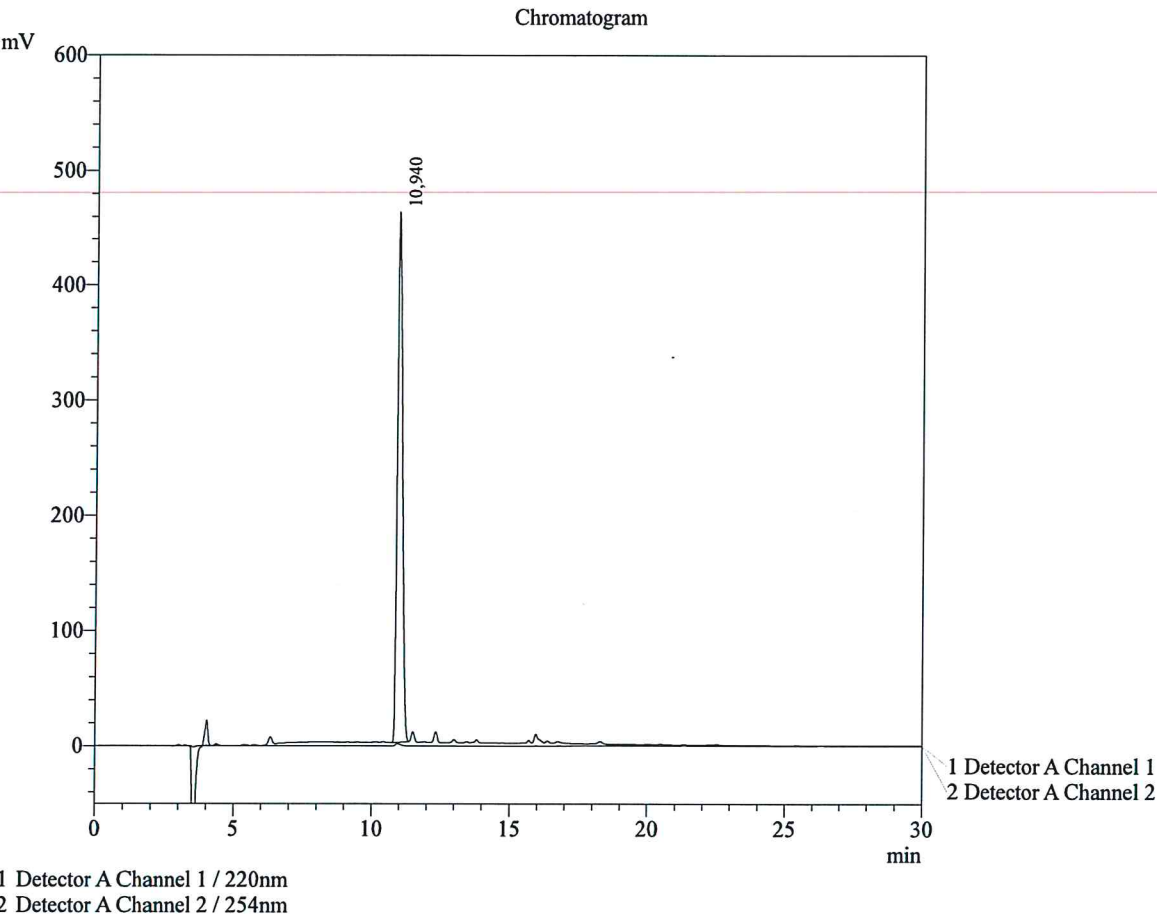

PeakTable			
Detector A Channel 1 220nm			
Peak#	Ret. Time	Area	Name
1	10,940	5707349	Argireline ®
Total			