

CERTIFICATE OF ANALYSIS

PRODUCT ARGIRELINE® peptide solution C
CODE P06-PD010
BATCH F885/20

ANALYTICAL BULLETIN

TEST	SPECIFICATION	RESULT	METHOD
Physical appearance	Translucent solution	Correct	CC-10-01-B6
Colour	Colourless	Correct	CC-10-01-B6
Specific gravity	-	-	-
pH	3.0-6.0	5.1	CC-10-01-B1
Viscosity (cPs) ¹	-	-	-
Particle size (mm)	-	-	-
Refractive index	-	-	-
Dry residue (%)	-	-	-
Identification (HPLC)	Similar retention time as in house ref. standard	Correct	CC-10-01-B19

MICROBIAL TEST

Total aerobic microbial count	<100 cfu/g	Correct	MI-10-01-D09
Total yeast and mould count	<10 cfu/g	Correct	MI-10-01-D09
<i>Escherichia coli</i>	Absence/g	Correct	MI-10-01-D09
<i>Pseudomonas aeruginosa</i>	Absence/g	Correct	MI-10-01-D09
<i>Staphylococcus aureus</i>	Absence/g	Correct	MI-10-01-D09
<i>Candida albicans</i>	Absence/g	Correct	MI-10-01-D09

Manufacturing date: 11/20
Retest date: 11/22

Approved on: 13/11/2020


QUALITY CONTROL
Anna Casadó

Printed on: 11/01/2021

QUALITY ASSURANCE
Dr. Fernando Fernández

FG-10-01/2 v.2

	Sample Information
Sample Name	: ARGIRELINE® peptide solution C
ID	: P06-PD010 F885/20
Data Filename	: 06112020P06-PD010.23.lcd
Date Acquired	: 08/11/2020 4:58:47
Column	: Kromasil 100-5C8, 250 x 4.6 mm

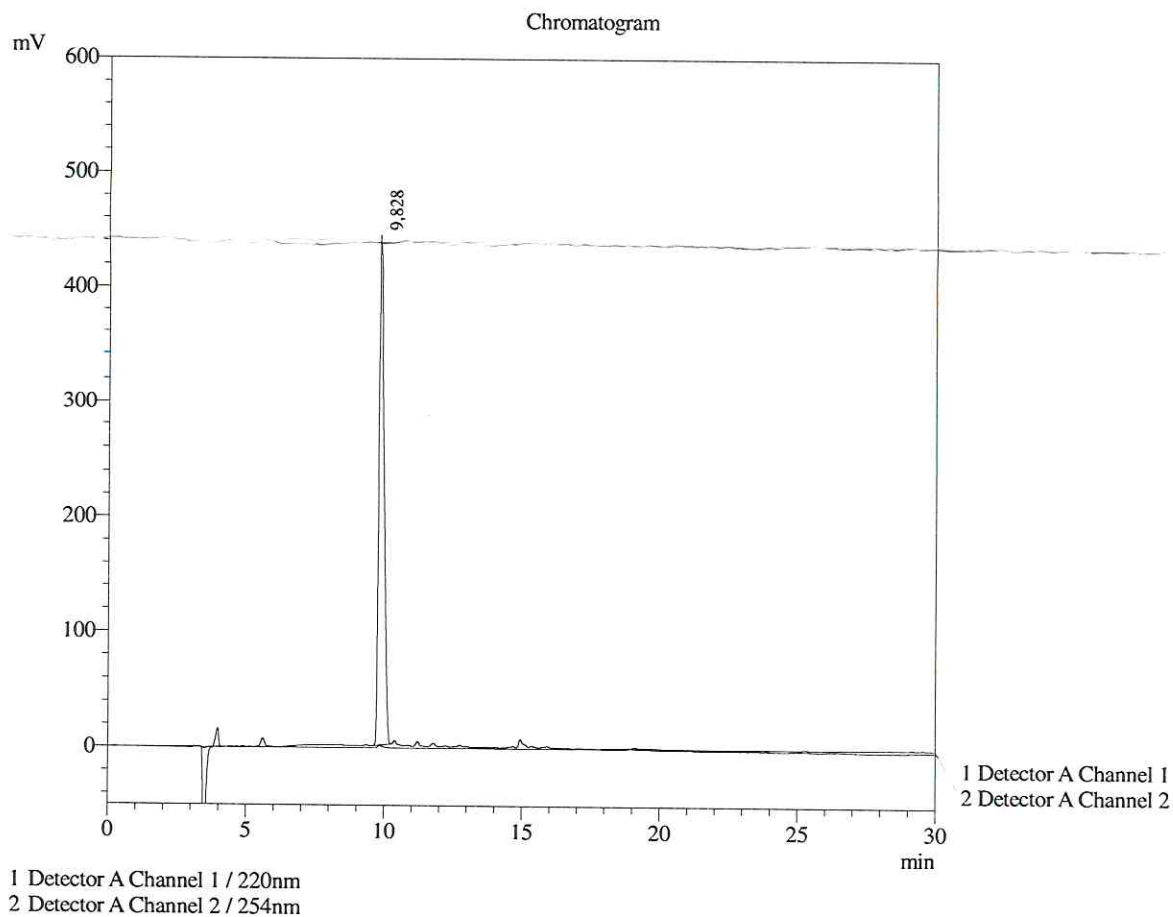

PeakTable

Peak#	Ret. Time	Area	Name
1	9,828	5740239	Argireline ®
Total			