

## CERTIFICATE OF ANALYSIS

PRODUCT ARGIRELINE® peptide solution C  
CODE P06-PD010  
BATCH F1090/20

### ANALYTICAL BULLETIN

| TEST                         | SPECIFICATION                                   | RESULT  | METHOD       |
|------------------------------|-------------------------------------------------|---------|--------------|
| Physical appearance          | Translucent solution                            | Correct | CC-10-01-B6  |
| Colour                       | Colourless                                      | Correct | CC-10-01-B6  |
| Specific gravity             | -                                               | -       | -            |
| pH                           | 3.0-6.0                                         | 5.0     | CC-10-01-B1  |
| Viscosity (cPs) <sup>1</sup> | -                                               | -       | -            |
| Particle size (mm)           | -                                               | -       | -            |
| Refractive index             | -                                               | -       | -            |
| Dry residue (%)              | -                                               | -       | -            |
| Identification (HPLC)        | Similar retention time as in house ref.standard | Correct | CC-10-01-B19 |

### MICROBIAL TEST

|                               |            |         |              |
|-------------------------------|------------|---------|--------------|
| Total aerobic microbial count | <100 cfu/g | Correct | MI-10-01-D09 |
| Total yeast and mould count   | <10 cfu/g  | Correct | MI-10-01-D09 |
| <i>Escherichia coli</i>       | Absence/g  | Correct | MI-10-01-D09 |
| <i>Pseudomonas aeruginosa</i> | Absence/g  | Correct | MI-10-01-D09 |
| <i>Staphylococcus aureus</i>  | Absence/g  | Correct | MI-10-01-D09 |
| <i>Candida albicans</i>       | Absence/g  | Correct | MI-10-01-D09 |

Manufacturing date: 01/21  
Retest date: 01/23

Approved on: 04/02/2021


QUALITY CONTROL  
Ana Poza

Printed on: 12/03/2021

QUALITY ASSURANCE  
Dr. Fernando Fernández

FG-10-01/2 v.2

|               |   |                                |
|---------------|---|--------------------------------|
|               |   | Sample Information             |
| Sample Name   | : | ARGIRELINE® peptide solution C |
| ID            | : | P06-PD010 F1090/20             |
| Data Filename | : | 25012021P06-PD010.109.lcd      |
| Date Acquired | : | 1/25/2021 7:59:15 PM           |
| Column        | : | Kromasil 100-5C8, 250 x 4.6 mm |

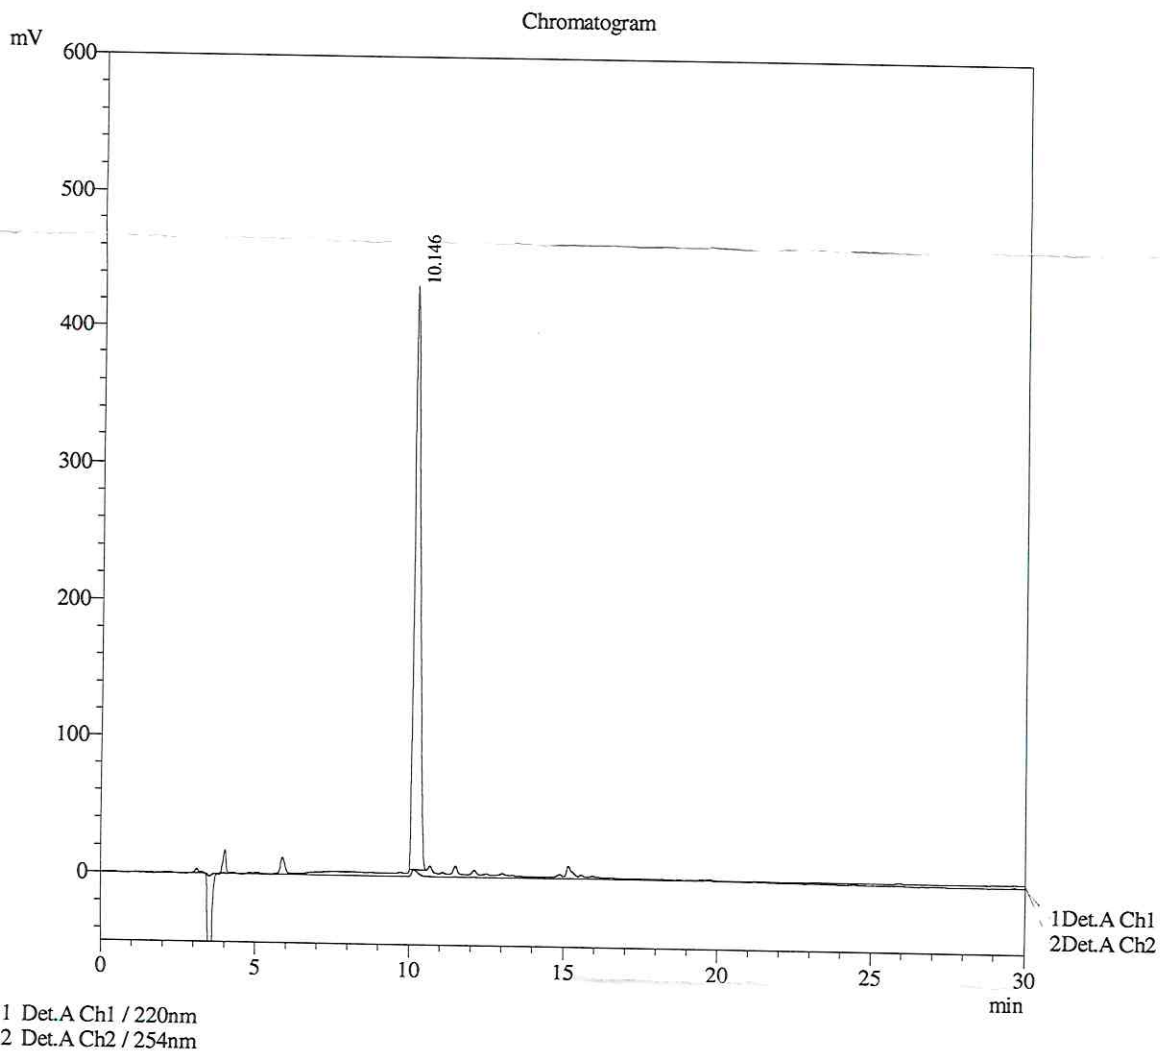

PeakTable

| Peak# | Ret. Time | Area    | Name |
|-------|-----------|---------|------|
| 1     | 10.146    | 5506072 |      |
| Total |           |         |      |