

CERTIFICATE OF ANALYSIS

PRODUCT ARGIRELINE® peptide solution C
CODE P06-PD010
BATCH F620/23

ANALYTICAL BULLETIN

TEST	SPECIFICATION	RESULT	METHOD
Physical appearance	Translucent solution	Correct	CC-10-01-B6
Colour	Colourless	Correct	CC-10-01-B6
Specific gravity	-	-	
pH	3.0-6.0	5.0	CC-10-01-B1
Viscosity (cPs) ¹	-	-	
Particle size (mm)	-	-	
Refractive index	-	-	
Dry residue (%)	-	-	
Identification (HPLC)	Similar retention time as in house ref.standard	Correct	CC-10-01-B19

MICROBIAL TEST

Total aerobic microbial count	<100 cfu/g	Correct	MI-10-01-D09
Total yeast and mould count	<10 cfu/g	Correct	MI-10-01-D09
<i>Escherichia coli</i>	Absence/g	Correct	MI-10-01-D09
<i>Pseudomonas aeruginosa</i>	Absence/g	Correct	MI-10-01-D09
<i>Staphylococcus aureus</i>	Absence/g	Correct	MI-10-01-D09
<i>Candida albicans</i>	Absence/g	Correct	MI-10-01-D09

Manufacturing date: 10/23

Retest date: 10/25

Approved on: 24/10/2023



QUALITY CONTROL
Ana Poza




QUALITY ASSURANCE
Dr. Fernando Fernández

Printed on: 14/12/2023

FG-10-01/2 v.2

Sample Information
Sample Name : ARGIRELINE® peptide solution C
ID : P06-PD010 F620/23
Data Filename : 18102023P06-PD010.005.lcd
Date Acquired : 18/10/2023 12:09:05
Column : Kromasil 100-5C8, 250 x 4.6 mm

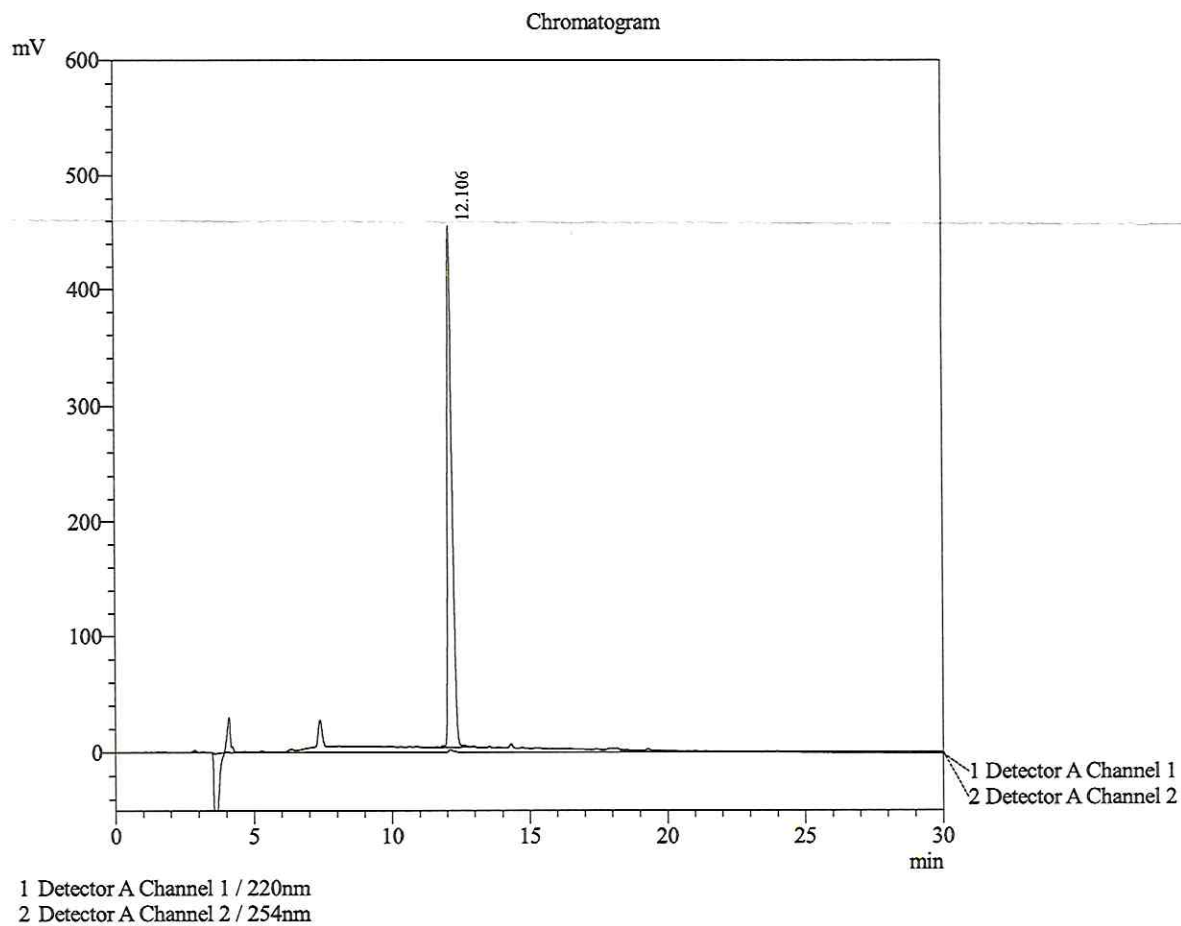

PeakTable

Detector A Channel 1 220nm			
Peak#	Ret. Time	Area	Name
1	12.106	5278361	Argireline ®
Total			