

CERTIFICATE OF ANALYSIS

PRODUCT ARGIRELINE® peptide solution C
CODE P06-PD010
BATCH F299/24

ANALYTICAL BULLETIN

TEST	SPECIFICATION	RESULT	METHOD
Physical appearance	Translucent solution	Correct	CC-10-01-B6
Colour	Colourless	Correct	CC-10-01-B6
Specific gravity	-	-	
pH	3.0-6.0	4.9	CC-10-01-B1
Viscosity (cPs) ¹	-	-	
Particle size (mm)	-	-	
Refractive index	-	-	
Dry residue (%)	-	-	
Identification (HPLC)	Similar retention time as in house ref.standard	Correct	CC-10-01-B19

MICROBIAL TEST

Total aerobic microbial count	<100 cfu/g	Correct	MI-10-01-D09
Total yeast and mould count	<10 cfu/g	Correct	MI-10-01-D09
<i>Escherichia coli</i>	Absence/g	Correct	MI-10-01-D09
<i>Pseudomonas aeruginosa</i>	Absence/g	Correct	MI-10-01-D09
<i>Staphylococcus aureus</i>	Absence/g	Correct	MI-10-01-D09
<i>Candida albicans</i>	Absence/g	Correct	MI-10-01-D09

Manufacturing date: 05/24

Retest date: 05/26

Released on: 03/06/2024



QUALITY CONTROL

Ana Poza




QUALITY ASSURANCE

Dr. Fernando Fernández

Printed on: 27/06/2024

FG-10-01/2 v.3

Sample Information	
Sample Name	: ARGIRELINE® peptide solution C
ID	: P06-PD010 F299/24
Data Filename	: 16052024P06-PD010.023.lcd
Date Acquired	: 16/05/2024 15:00:06
Column	: Kromasil 100-5C8, 250 x 4.6 mm

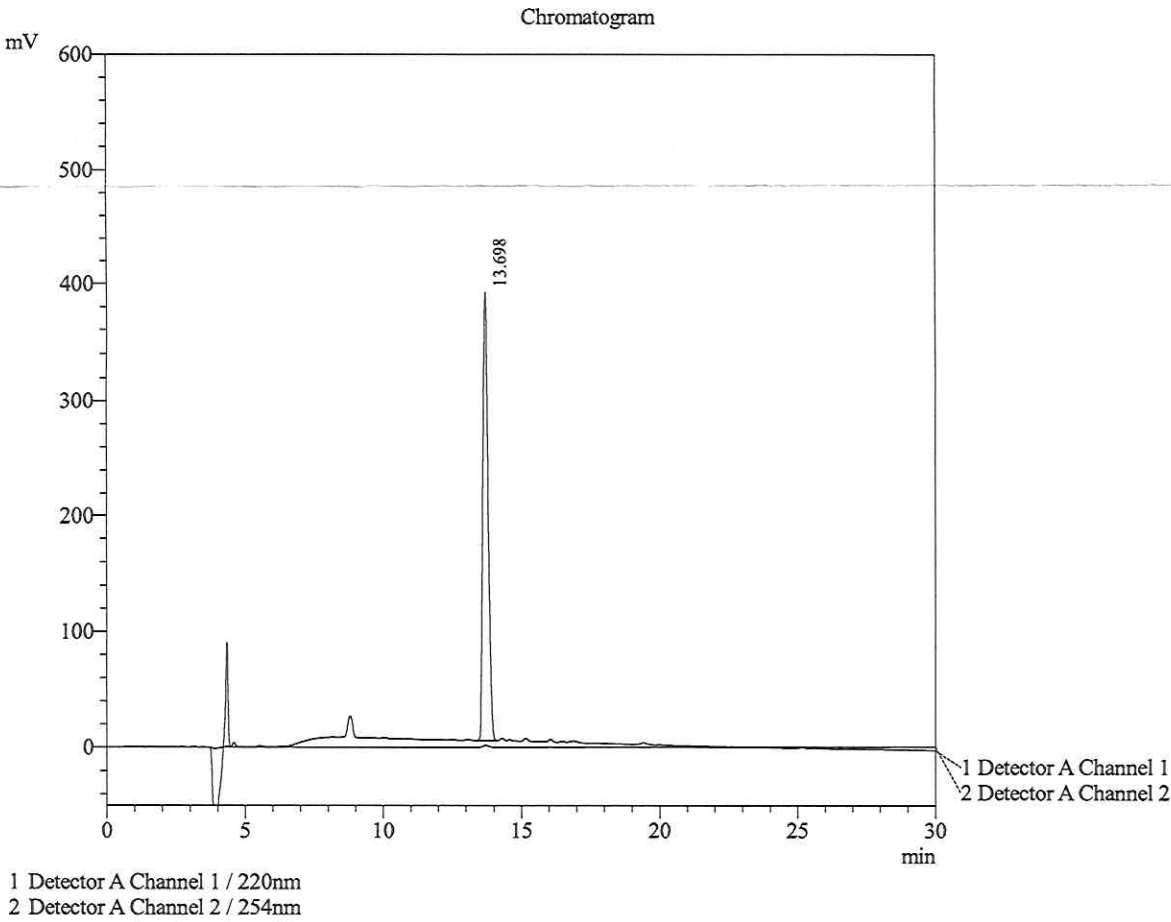

PeakTable			
Detector A Channel 1 220nm			
Peak#	Ret. Time	Area	Name
1	13.698	5084742	Argireline ®
Total			