


Certificate of Analysis – Certified Reference Material

PROGESTERONE

Product no.: PHR1142-1G
Lot no.: LRAD7358
Description of CRM: White Powder
Expiry date: 31 May 2028
Storage: 2°C to 30 °C/Protect from Light
Certificate version: LRAD7358.1 (Note: Certificates may be updated due to Pharmacopeial Lot Changes or the availability of new data. Check our website at: www.sigma-aldrich.com for the most current version.)
Chemical formula: C₂₁H₃₀O₂
Molecular mass: 314.46
CAS No.: 57-83-0

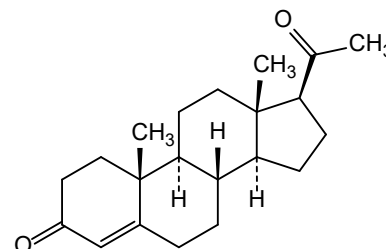

Analyte	Certified Purity ± associated uncertainty U , $U = k \cdot u$ ($k = $) (qNMR/ basis)
PROGESTERONE	99.3 % U _{crm} = ± 0.4 %, $k = 2.0$ (as is basis)

Metrological traceability: Traceable to the SI and higher order standards from NIST through an unbroken chain of comparisons. Additional traceability to Primary Standards is established through comparative assay determinations. See "Details on metrological traceability" on page 2.
Measurement method: Where applicable, the certified value is based on a purity determination by mass balance. See "Certification process details" on page 3.
Intended use: Intended for R&D and Analytical Use only. Not for drug, household or other uses
Minimum sample size: 20 mg
Instructions for handling and correct use: Do not dry, use on the as is basis. The internal pressure of the container may be slightly different from the atmospheric pressure at the user's location. Open slowly and carefully to avoid dispersion of the material. Attachment of a 20 mm aluminum crimp seal recommended for unused portions.
Health and safety information: All chemical reference materials should be considered potentially hazardous and should be used only by qualified laboratory personnel. Please refer to the Safety Data Sheet for detailed information about the nature of any hazard and appropriate precautions to be taken.
Accreditation: Sigma-Aldrich RTC is accredited by the US accreditation authority ANAB as a registered reference material producer AR-1470 in accordance with ISO 17034.
Certificate issue date: 31 May 2024



[Andy Ommen; Quality Control]

Shawn Stetler- QA Manager



Packaging: 1 g in amber vial

Details on metrological traceability:

This standard has been gravimetrically prepared using balances that have been fully qualified and calibrated to ISO 17025 requirements. All calibrations utilize NIST traceable weights which are calibrated externally by a qualified ISO 17025 accredited calibration laboratory to NIST standards. Qualification of each balance includes the assignment of a minimum weighing by a qualified and ISO 17025 accredited calibration vendor taking into consideration the balance and installed environmental conditions to ensure compliance with USP tolerances of NMT 0.10% relative error. Fill volume to predetermined specifications is gravimetrically verified throughout the dispensing process using qualified and calibrated balances. Further traceability to a corresponding Primary Standard may be achieved through a direct comparison assay. Where a Primary Standard is available, the assay value will be included in the specified section of the COA.

Associated uncertainty:

Uncertainty values in this document are expressed as Expanded Uncertainty (U_{CRM}) corresponding to the 95% confidence interval. U_{CRM} is derived from the combined standard uncertainty multiplied by the coverage factor k , which is obtained from a t -distribution and degrees of freedom. The components of combined standard uncertainty include the uncertainties due to characterization, homogeneity, long term stability, and short term stability (transport). The components due to stability are generally considered to be negligible unless otherwise indicated by stability studies.

$$U_{crm} = \left(\sqrt{u_{characterization}^2 + u_{homogeneity}^2 + u_{stability}^2} \right) \times k$$

Traceability Assay:

Comparative assay demonstrates direct traceability to Pharmacopeial Standards

ASSAY vs. USP REFERENCE STANDARD (1568007) (as is basis)

ASSAY VALUE

99.4 %

vs. USP LOT

R15550

Labeled Content = 0.999 mg/mg

ASSAY vs. EP CRS (P3300000) (as is basis)

ASSAY VALUE

99.7 %

vs. EP BATCH

5.0

Labeled Content = 99.6 %

ASSAY vs. BP CRS (449) (as is basis)

ASSAY VALUE

99.3 %

vs. BP BATCH

4181

Labeled Content = 99.2 %

METHOD: HPLC (ref.: Progesterone, Current Compendial Monographs)

Column: Ascentis Express C18 150 x 4.6mm, 5µm particle size

Mobile Phase A: Water

Mobile Phase B: Acetonitrile

Gradient:

Time (min)	%A	%B
0-20	50	50
27-45	20	80
45.1-55	50	50

Flow Rate: 1.0 mL/min

Column Temperature: 30 °C

Injection Volume: 10 µL

Detector: DAD, Wavelength: 241 nm

Representative Chromatogram from Lot: LRAD7358 Analysis



CHROMATOGRAPHIC IMPURITY ANALYSIS

METHOD: HPLC (ref.: Progesterone, Current Compendial Monographs)

See HPLC Assay


Detector: DAD, Wavelengths: 241 nm and 286 nm

Impurities Detected


Impurity B:	0.063 %	Impurity C:	0.24 %
Impurity G:	0.065 %	Impurity H:	0.10 %

Total Impurities: **0.47 %**

Representative Chromatogram from Lot: LRAD7358 Impurity 241 nm Analysis

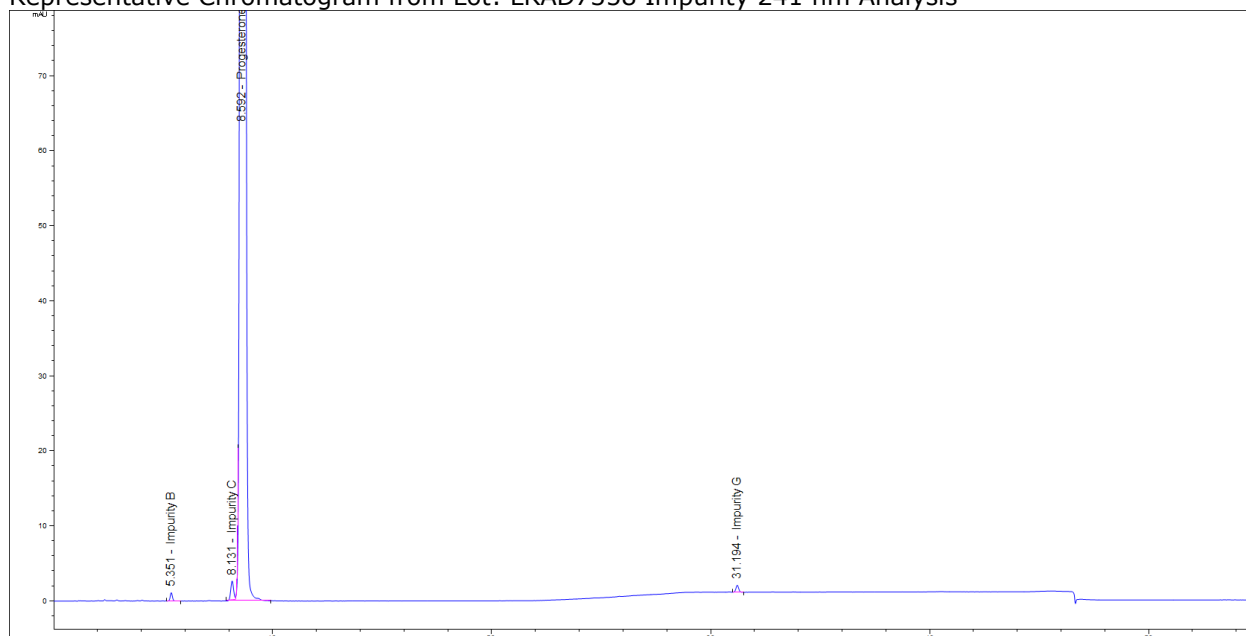

Representative Chromatogram from Lot: LRAD7358 Impurity 286 nm Analysis

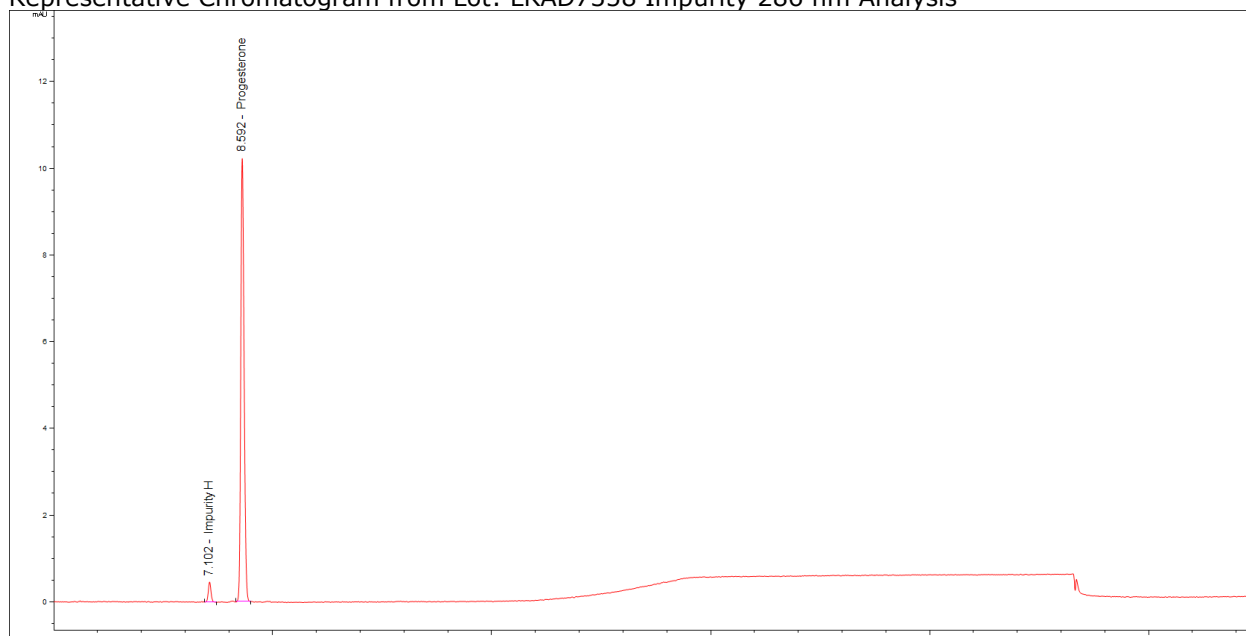

LOSS ON DRYING/VOLATILES

Method: Under vacuum over silica gel for 4 hours (ref.: Current Compendial Monographs)

Mean of three measurements, Loss = **None**

RESIDUE ANALYSIS

Method: Sulfated Ash (ref.: Current Compendial Monographs)

Sample Size: ~ 300 mg

Mean of three measurements, Residue = **None**

Certification process details:

The certified purity is determined by qNMR and calculated as

$$P_{\text{Sample}} = \frac{I_{\text{Analyte}}}{I_{\text{CRM}}} \cdot \frac{N_{\text{CRM}}}{N_{\text{Analyte}}} \cdot \frac{M_{\text{Analyte}}}{M_{\text{CRM}}} \cdot \frac{m_{\text{CRM}}}{m_{\text{Sample}}} \cdot P_{\text{CRM}}$$

- P_{Sample} Purity of samples as mass fraction (%)
- P_{CRM} Purity of CRM as mass fraction (%)
- I_{Analyte} Integral of the analyte signal
- I_{CRM} Integral of CRM signal
- N_{Analyte} Number of analyte nuclei
- N_{CRM} Number of CRM nuclei
- M_{Analyte} Molecular mass of the analyte (g/mol)
- M_{CRM} Molecular mass of the CRM (g/mol)
- m_{Sample} Mass of sample (mg)
- m_{CRM} Mass of CRM (mg)

CERTIFIED PURITY BY qNMR (Mass Fraction, n = 9)

99.3 % $U_{\text{CRM}} = \pm 0.4 \%$, $k = 2.0$
(as is basis)

METHOD: quantitative NMR spectroscopy

Condition: Bruker 500 MHz

Solvent: DMSO- d_6

Internal standard: 1,3,5-Trimethoxybenzene (TraceCERT: 74599)

Homogeneity assessment: Homogeneity was assessed in accordance with ISO Guide 35. The material is tested by qNMR measurements using 4 or 9 subsamples which are taken from different positions in the entire bulk material. The recommended minimal sample size is taken for all the homogeneity test samples. Analysis of variance (ANOVA) result are included into the calculation of content uncertainty of this CRM.

Analytical method: qNMR


Sample size: 20 mg

Stability assessment: Significance of the stability assessment will be demonstrated if the analytical result of the study and the range of values represented by the Expanded Uncertainty do not overlap the result of the original assay and the range of its values represented by the Expanded Uncertainty. The method employed will usually be the same method used to characterize the assay value in the initial evaluation.

Long Term Stability Evaluation - An assessment, or re-test, versus a Compendial Reference Standard may be scheduled, within the 3 year anniversary date of a release of a Secondary Standard. The re-test interval will be determined on a case-by-case basis. Short Term Stability Study - It is useful to assess stability under reasonably anticipated, short term transport conditions by simulating exposure of the product to humidity and temperature stress. This type of study is conducted under controlled conditions of elevated temperature and humidity.

Identification Test:

INFRARED SPECTROPHOTOMETRY (Comparative identification analysis demonstrates direct traceability to Pharmacopeial standards)

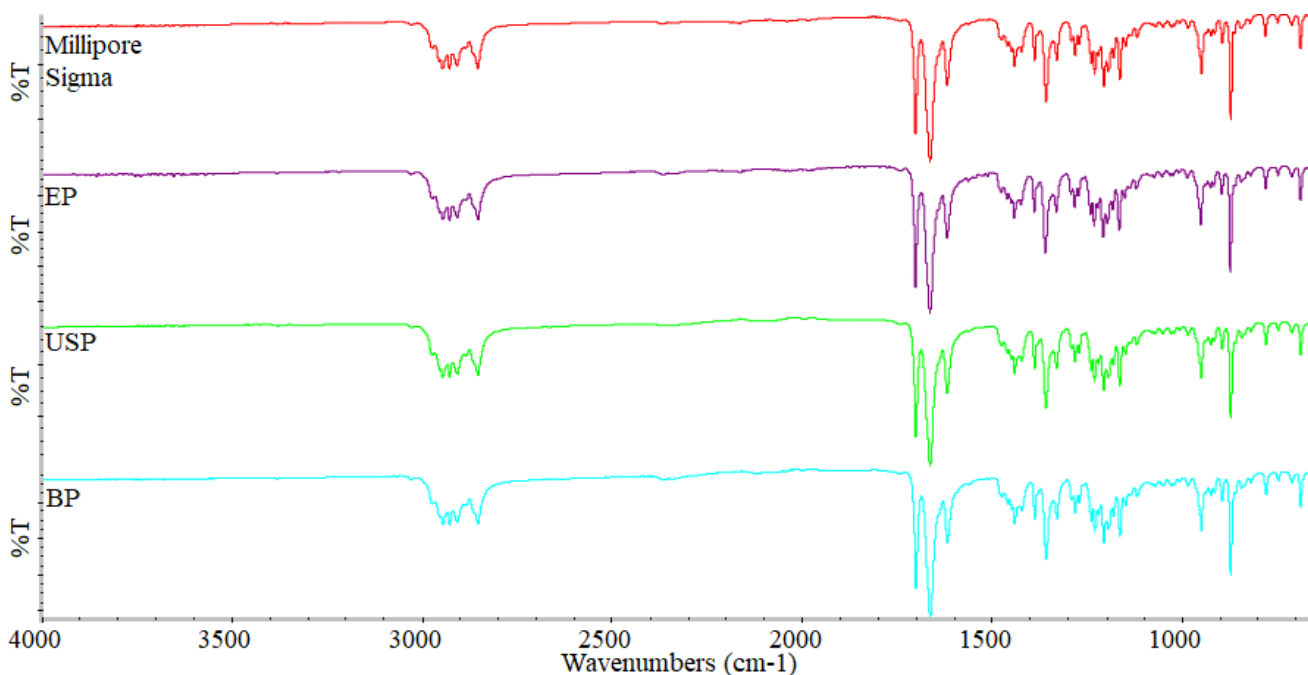


MilliporeSigma Lot: LRAD7358 vs EP Batch: 5.0 / USP Lot: R15550 / BP Batch: 4181

Indicative Values:

MASS SPECTRUM


Method: HR-QTOF; 4.0 kV ESI+; temperature: 325 °C

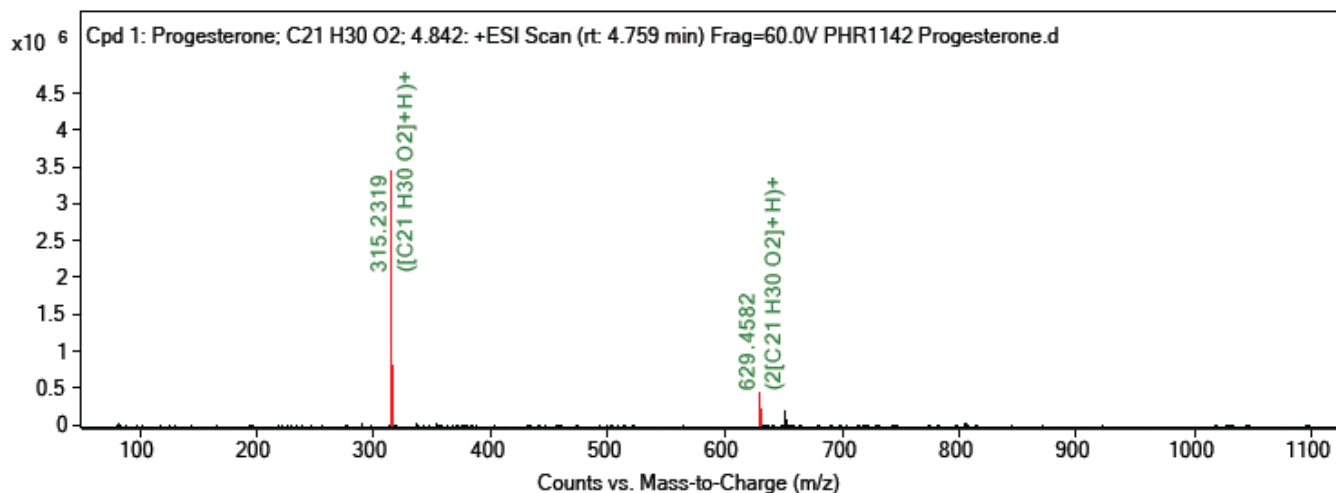

Theoretical value: 315.2324 m/z


The signal of the MS spectrum is consistent with the theoretical value and its interpretation is consistent with the structural formula.

¹H NMR

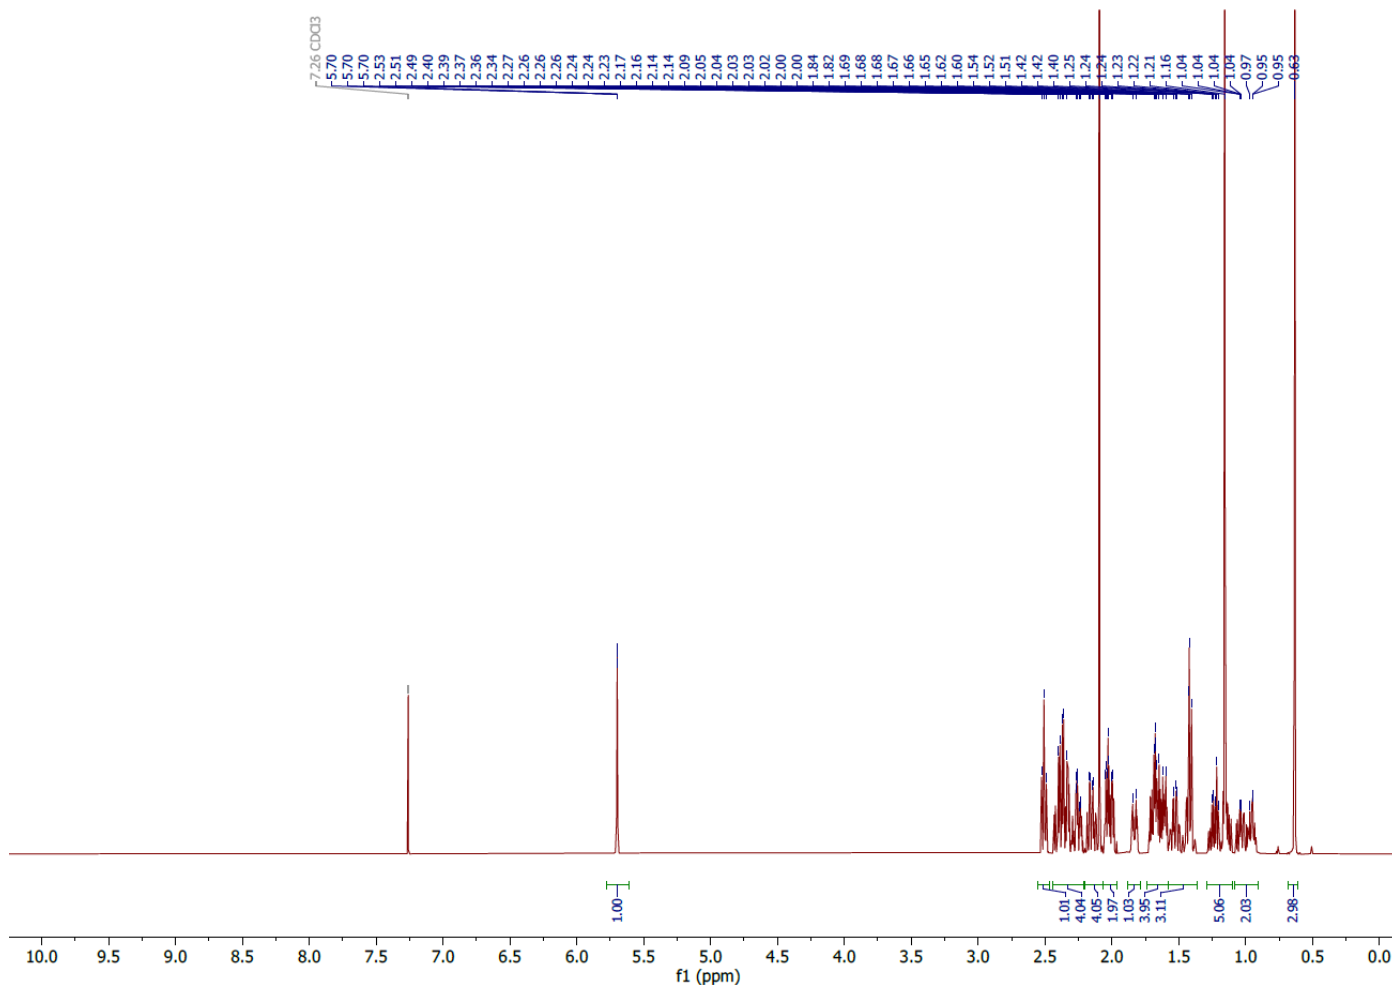

Consistent with structure

Quantitative NMR Spectrum

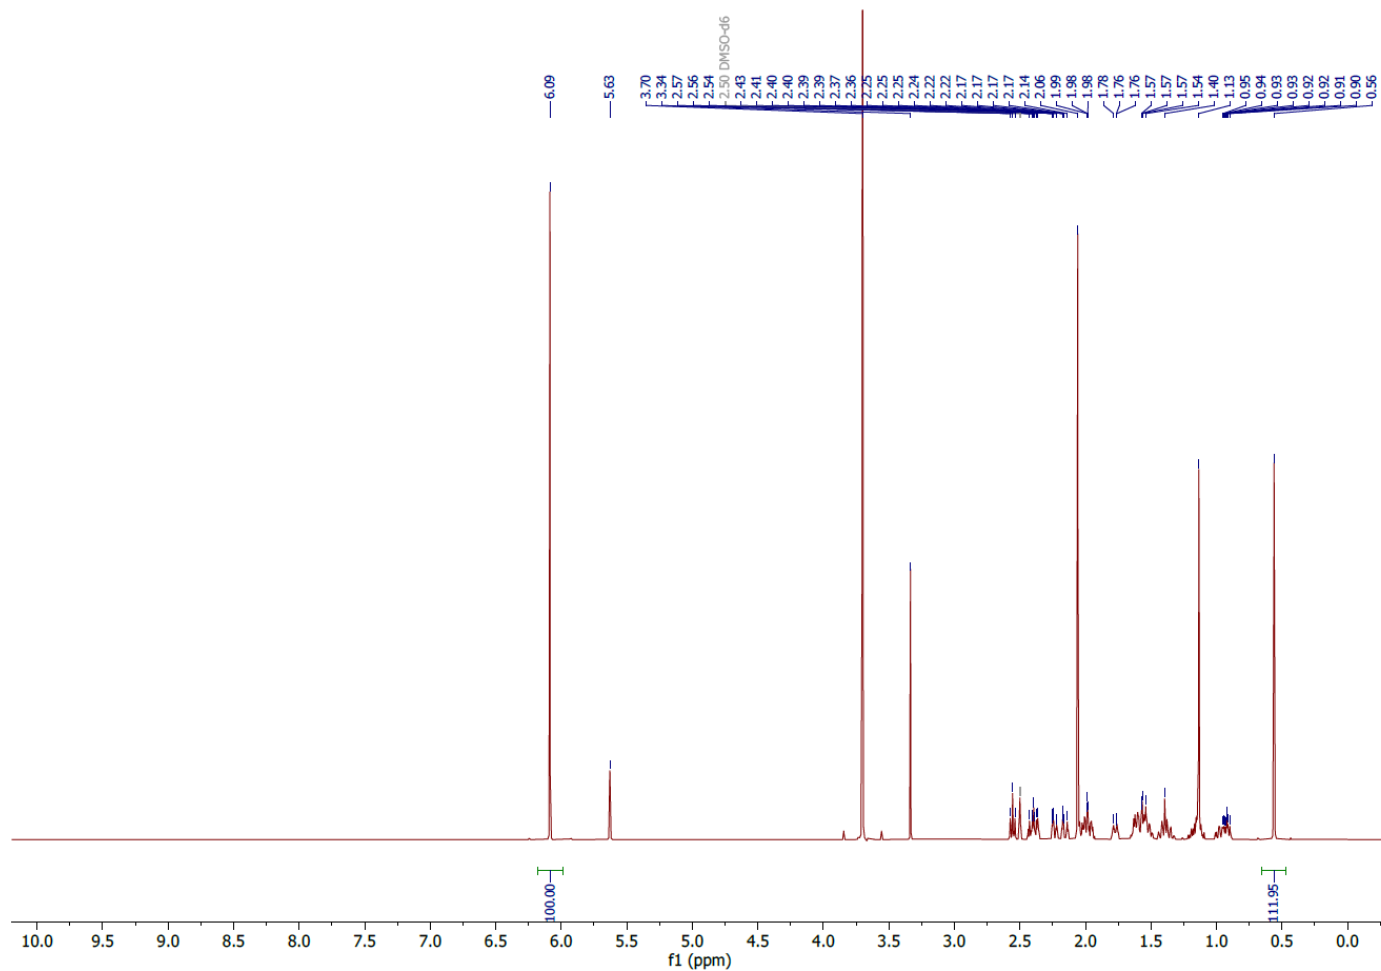

MELTING RANGE

Specification: Between 126 and 131°C (USP)

Buchi M-565

Mean of three measurements = **128.8 – 130.1 °C**

OPTICAL ROTATION

Specification: Specific Rotation between +175 and +183 (USP)

Perkin Elmer Polarimeter 343

Wavelength: 589nm

Concentration: 200mg/10mL in dioxane

Cell Path: 100mm

Mean of three Measurements = **+181.83**

Certificate of analysis revision history:

Certificate version	Date	Reason for version
LRAD7358.1	31 May 2024	Original Release

Disclaimer:

The purchaser is required to determine the suitability of this product for any particular application. Sigma-Aldrich RTC makes no warranty of any kind, express or implied, other than its products meet all quality control standards set by Sigma-Aldrich RTC. We do not guarantee that the product can be used for any particular application.

The vibrant M, Supelco, TraceCERT and Sigma-Aldrich are trademarks of Merck KGaA, Darmstadt, Germany or its affiliates. All other trademarks are the property of their respective owners. Detailed information on trademarks is available via publicly accessible resources.
© 2018 Merck KGaA, Darmstadt, Germany and/or its affiliates. All Rights Reserved.

The life science business of Merck KGaA, Darmstadt, Germany operates as MilliporeSigma in the US and Canada.

