

CERTIFICATE OF ANALYSIS

PRODUCT ARGIRELINE[®] SOLUTION C
CODE P06-PD010
BATCH F885/12
DATE 21/09/12

ANALYTICAL BULLETIN

TEST	SPECIFICATION	RESULT	METHOD
APPEARANCE	TRANSLUCENT SOLUTION	CORRECT	CC-10-01-B6
COLOUR	COLOURLESS	CORRECT	CC-10-01-B6
SPECIFIC GRAVITY (g/ml)	N.A.		
pH	3.0 – 6.0	4.6	CC-10-01-B1
VISCOSITY (cPs)	N.A.		
PARTICLE SIZE (mm)	N.A.		
REFRACTIVE INDEX	N.A.		
DRY RESIDUE (%)	N.A.		
IDENTIFICATION (HPLC)	SIMILAR RETENTION TIME AS IN HOUSE REF. STANDARD	CORRECT	CC-10-01-B19

MICROBIAL TEST

TOTAL AEROBIC MICROBIAL COUNT	< 100 cfu/g.	CORRECT	USP 35
TOTAL YEAST AND MOULD COUNT	< 10 cfu/g	CORRECT	USP 35
SPECIFIC MICROORGANISMS:			
<i>Escherichia Coli</i>	ABSENCE/0.5g	CORRECT	USP 35
<i>Pseudomonas Aeruginosa</i>	ABSENCE/g	CORRECT	USP 35
<i>Staphylococcus Aureus</i>	ABSENCE/g	CORRECT	USP 35
<i>Candida Albicans</i>	ABSENCE/g	CORRECT	USP 35

REMARKS

MANUFACTURING DATE 10/12
RETEST DATE 10/14


QUALITY CONTROL
Dra. Gemma Jodas

QUALITY ASSURANCE
Dra. Laia González

This Certificate of Analysis has been produced electronically and is valid without signature

FG-10-01/2 (version,1)

Sample Information
 Sample Name : ARGIRELINE® SOLUTION C
 ID : P06-PD010 F885/12
 Data Filename : 101012F88512.005.lcd
 Date Acquired : 09/10/2012 15:22:32
 Column : Kromasil 100-5C8, 250 x 4.6 mm

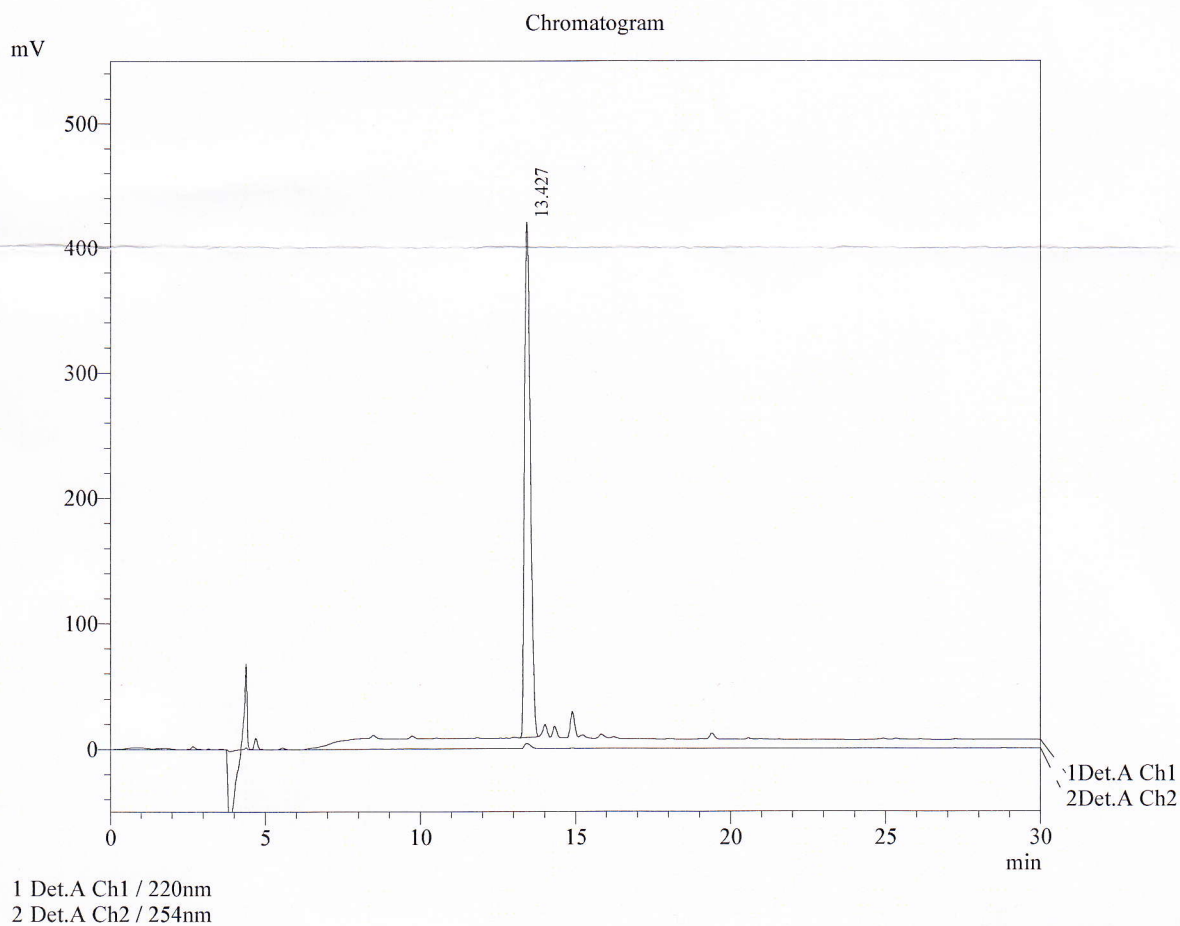

PeakTable

Peak#	Ret. Time	Area	Name
1	13.427	5332872	Argireline ®
Total			